
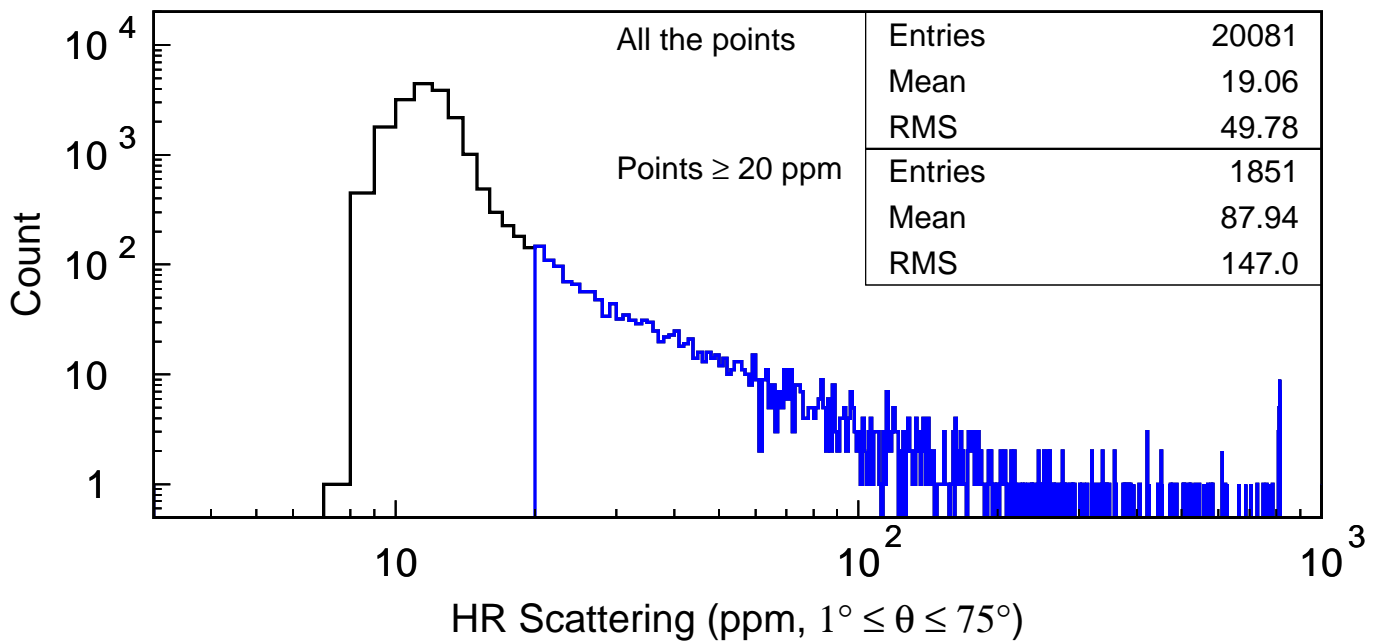




ETM11 HR TIS measurement, 111121

($\phi_{\text{beam}} = 0.3 \text{ mm}$, Step = 1.0 mm)

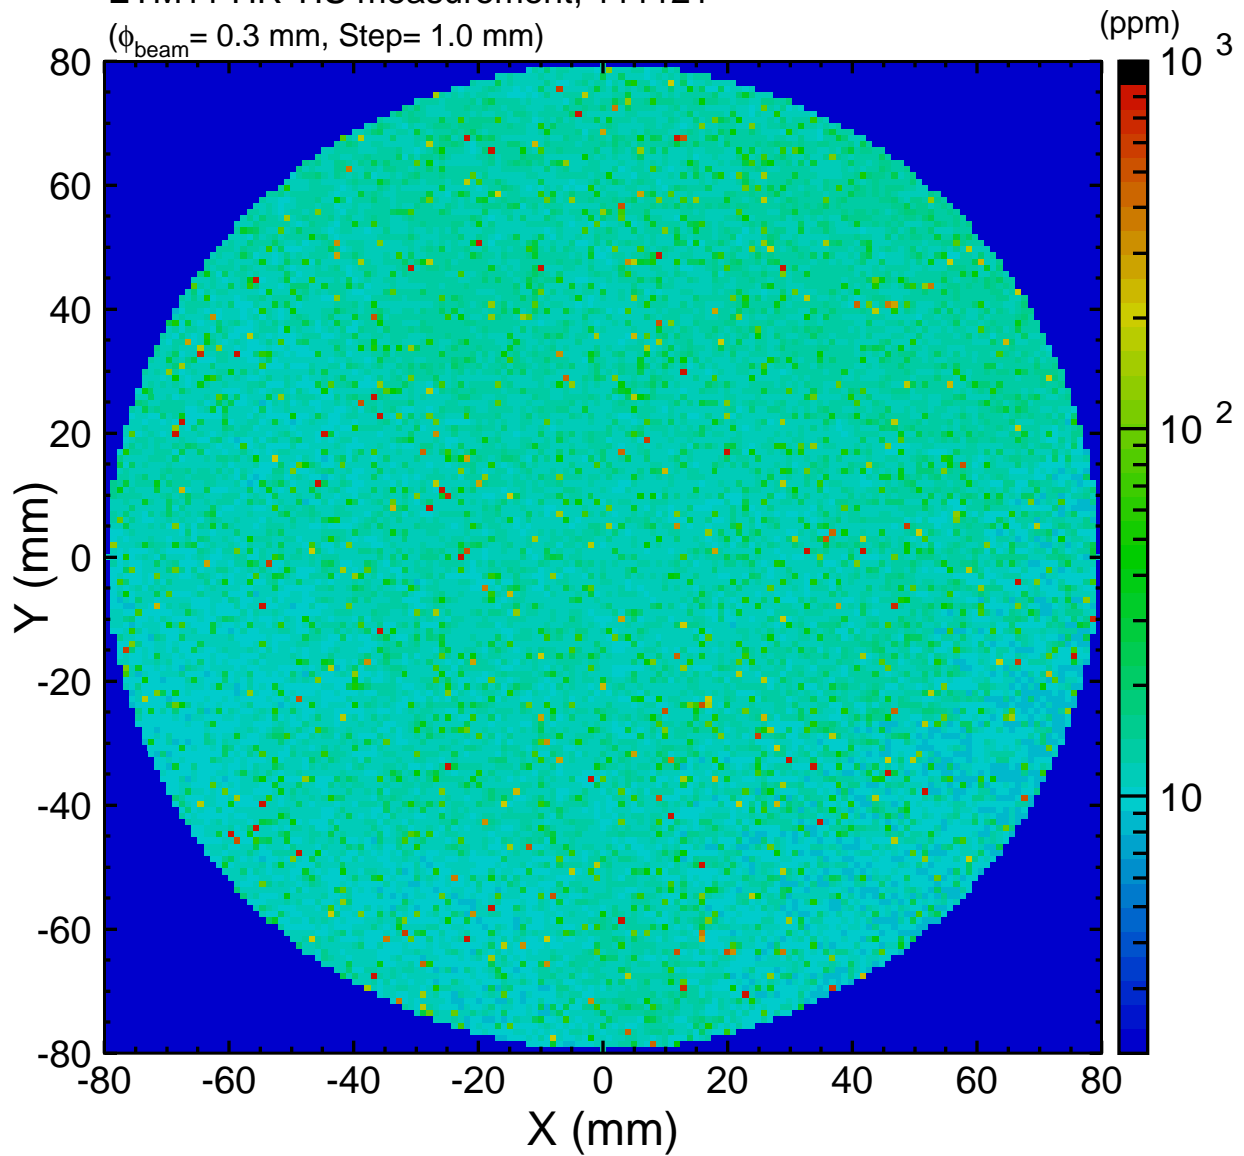

ETM11 HR TIS measurement, 111321

($\phi_{\text{beam}} = 0.3 \text{ mm}$, Step= 0.3 mm)

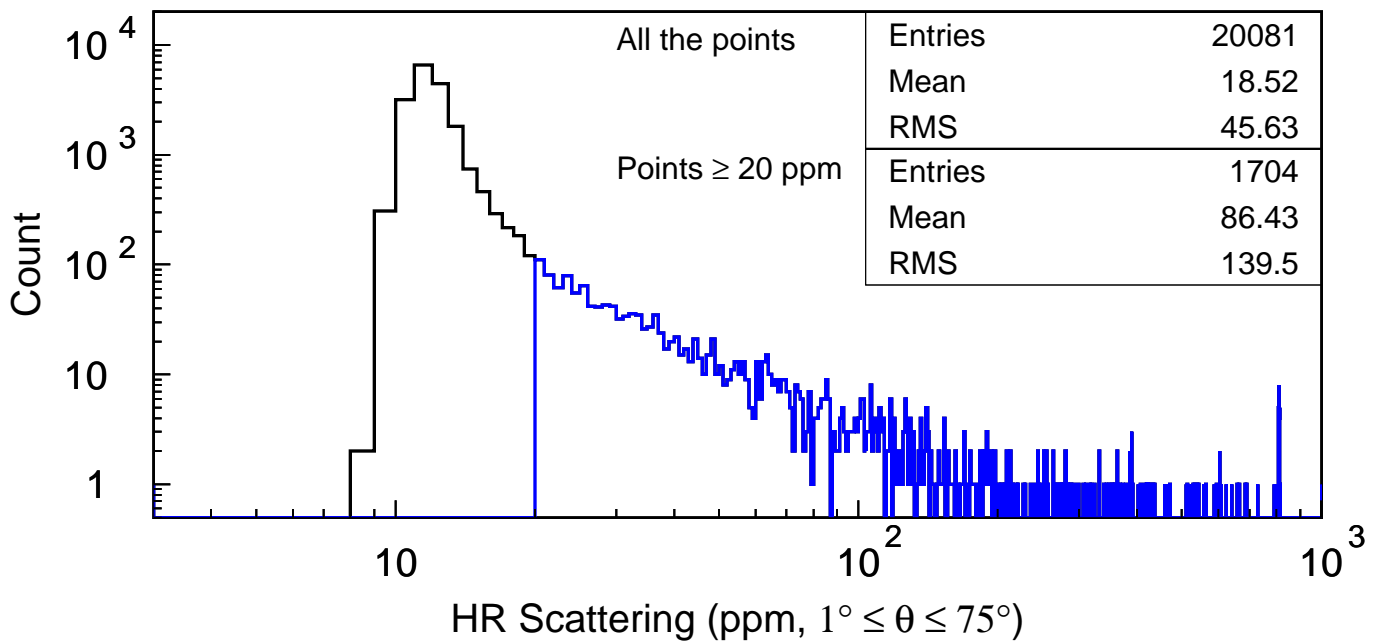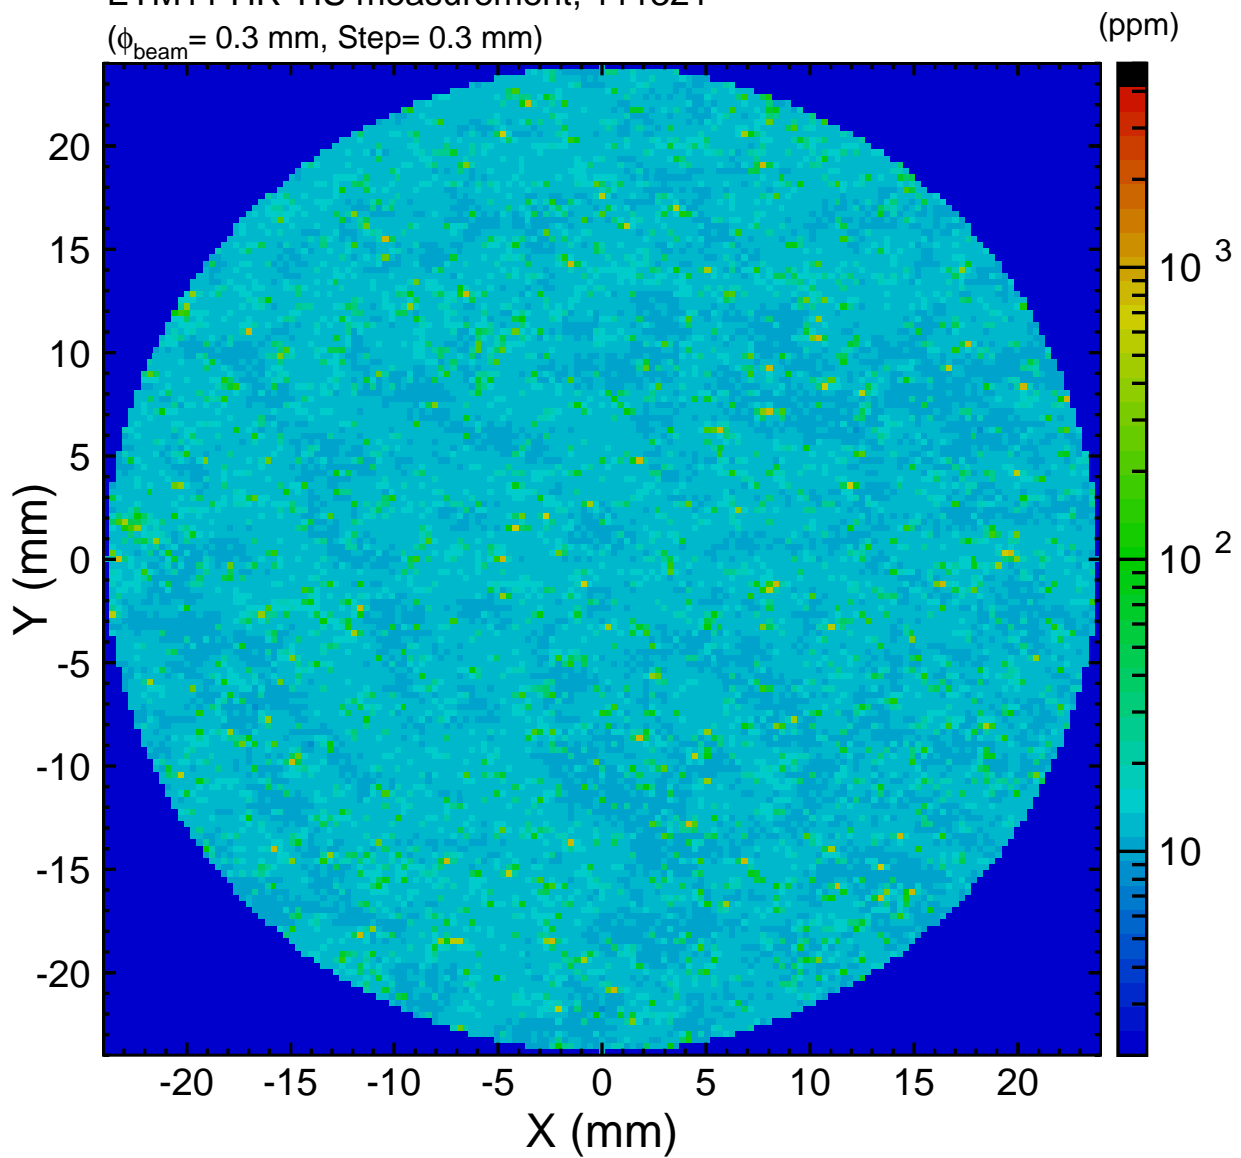

ETM11 HR TIS measurement ($\phi_{\text{beam}} = 0.3 \text{ mm}$, Step= 0.3 mm)

